
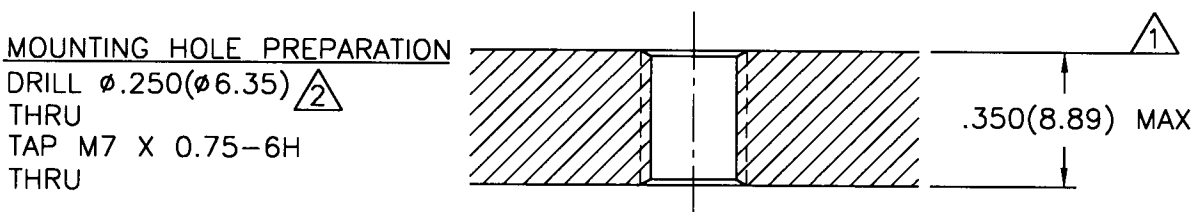


APPLICATION		
NEXT ASS'Y	USED ON	VAR

REVISIONS				
REV	DESCRIPTION	ECN	DATE	APP'D
A	REVISED PER ECN	6228	11-28-95	DM/qr

2571
PCB Piezotronics Inc. claims proprietary rights in the information disclosed hereon. Neither it nor any reproduction thereof will be disclosed to others without written consent of PCB Piezotronics Inc.

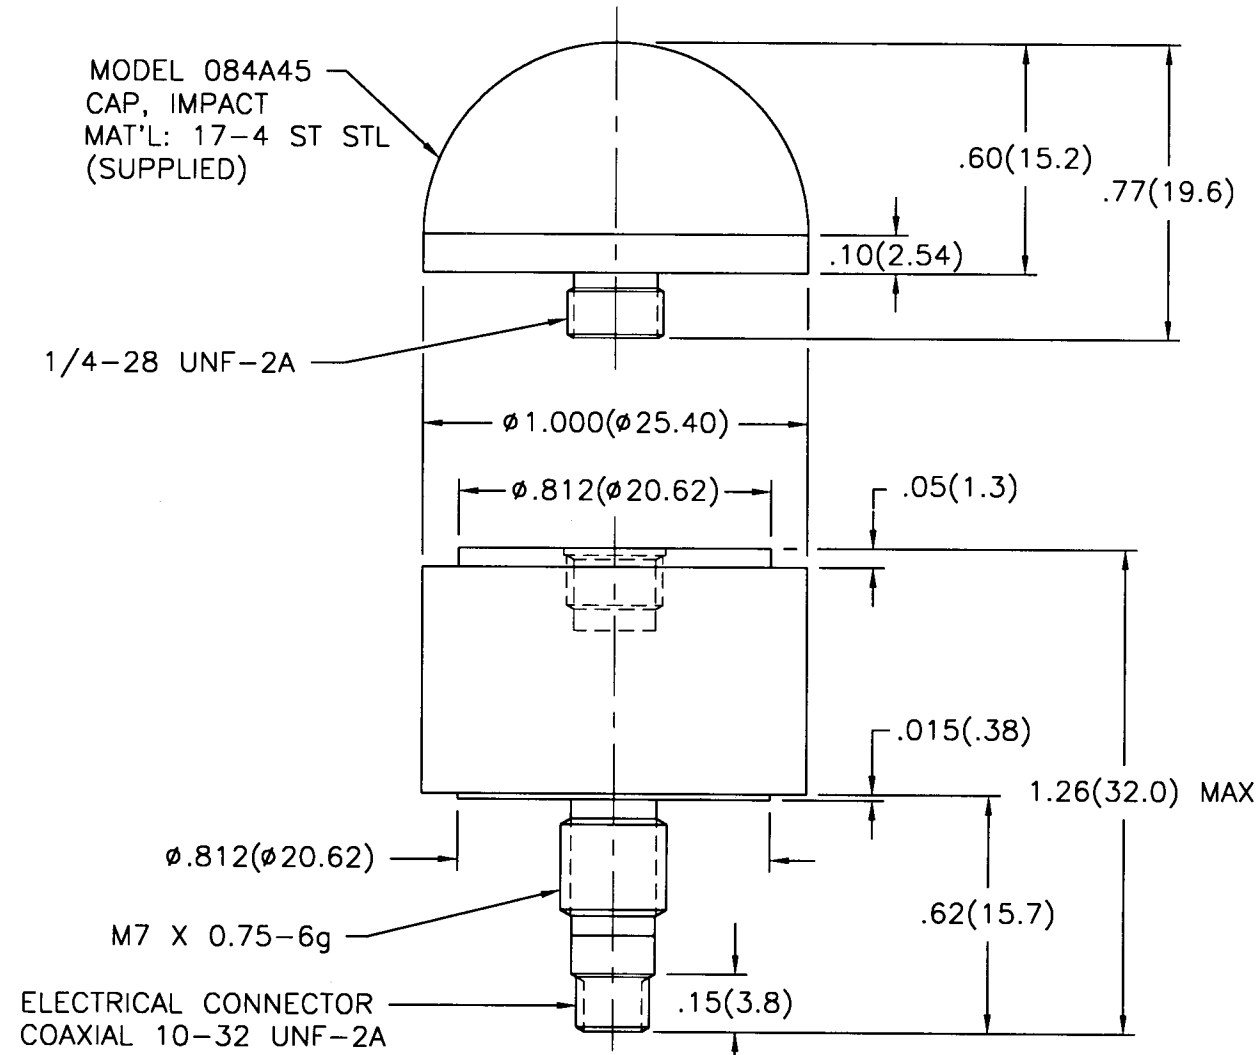

- 3.) RECOMMENDED MOUNTING TORQUE 20-24 IN LBS (226-271 NEWTON CENTIMETERS).
- $\triangle 2$ DRILL PERPENDICULAR TO MOUNTING SURFACE TO WITHIN $\pm 1^\circ$.
- $\triangle 1$ MOUNTING SURFACE UNDER TRANSDUCER MUST BE FLAT WITHIN .001(0.03) TIR OVER A $\phi .812(\phi 20.60)$ MIN WITH A $63\sqrt{1.6}$ FINISH.

UNLESS SPECIFIED TOLERANCES		DRAWN	<i>ZUB</i>	MFG	<i>11/28/95</i>	PCB PIEZOTRONICS, INC. 3425 WALDEN AVE. DEPEW, NEW YORK 14043 PHONE: (716) 684-0001
DIMENSIONS IN INCHES	DIMENSIONS IN MILLIMETERS (IN PARENTHESIS)	CHK'D	<i>DM</i>	ENGR	<i>P.M.</i>	
DECIMALS XX \pm .01 XXX \pm .005	DECIMALS XX \pm 0.3 XXX \pm 0.13	APP'D	<i>DM</i>		<i>11/29/95</i>	
ANGLES \pm 2 DEGREES	ANGLES \pm 2 DEGREES	TITLE	INSTALLATION DRAWING MODEL 208A45 FORCE TRANSDUCER			
FILLETS AND RADII .003 - .005	FILLETS AND RADII (0.07 - 0.13)	CODE IDENT. NO.	52681		DWG. NO.	2571
DD011 REV. A 05/26/95		SCALE: 2X		SHEET 1 OF 1		